


Aria Shutdown Guide

1

Run Bleach for 2-3 minutes to sterilize machine.

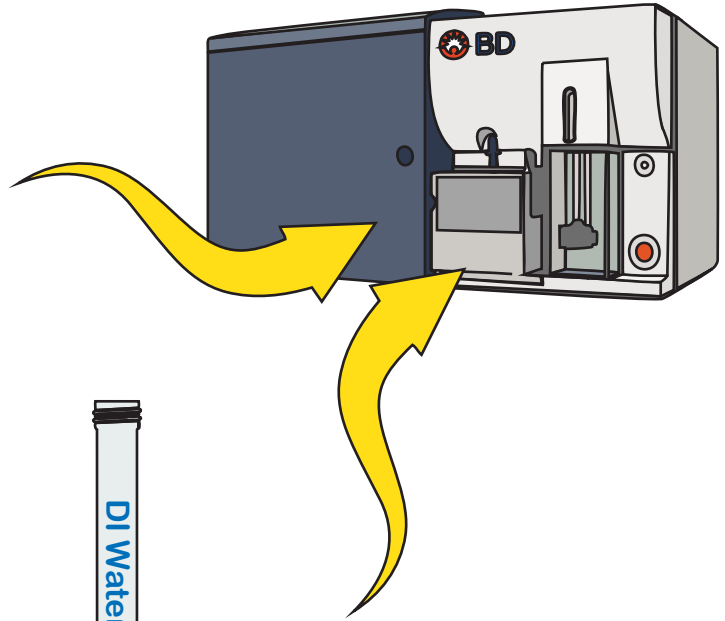


2

Run DI Water for 2-3 minutes to clean machine.




3

Turn the Stream off in the software.

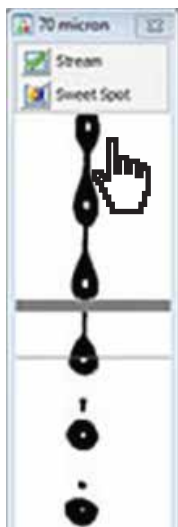

4


Push the Power Button on the left side of the machine.

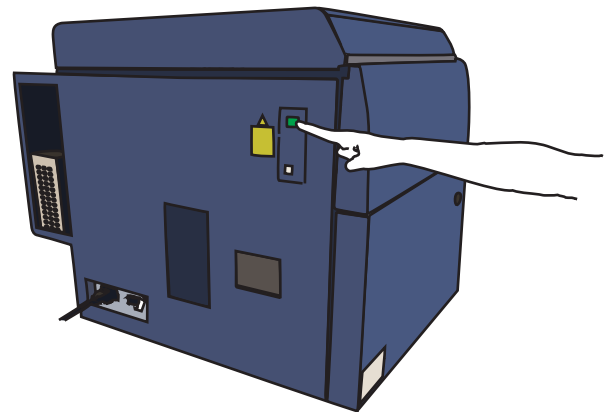

5

Turn off the Air Valve. Turn the handle so it is perpendicular to the copper pipe.

The Aria 594 air valve is located to the left on the counter

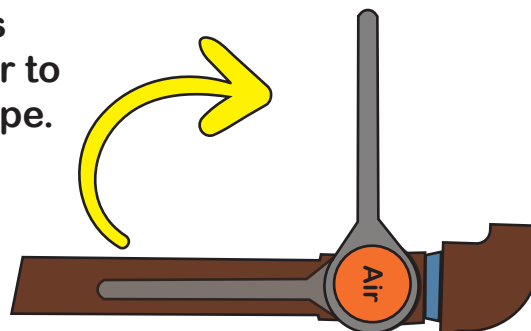

The Aria 561 air valve is located to the right on the wall



**Harvard Medical School
Immunology Flow Core**